

# Why ventilate and heat pyranometers

Required for all high-accuracy measurements: improve data availability and reduce zero offset errors

*Ventilation of pyranometers has always been recommended by WMO, ISO and ASTM to reduce the effects of dew and frost, and to reduce zero offset errors. Now it is also a requirement for Class A systems for PV system performance monitoring according to IEC 61724-1. Hukseflux recommends all high accuracy measurements, aiming at a measurement accuracy of better than 5 %, to be equipped with heating and ventilation. It is important to also be aware of the shortcomings of ventilation. Ventilation is NOT a way to reduce instrument maintenance or cleaning interval. Ventilation is seldom effective to remove snow.*

## Introduction

In most climates deposition of dew and frost causes significant errors when measuring solar radiation. In particular in the early morning before instruments can be manually cleaned. Just heating a pyranometer is not an option; it produces large zero offsets in a pyranometer thermal detector.

## Hukseflux' recommendation in summary

Hukseflux recommends to heat and ventilate either using SR30 with "recirculating ventilation and heating" (Figure 1) or an external ventilation system such as VU01 with pyranometer SR20 (Figure 3):

- if you aim for a measurement accuracy of better than 5 % ( $k = 2$ )
- in all arctic conditions with regular frost
- if you work in utility scale PV monitoring according to IEC 61724-1 Class A

What not to do:

- use VU01 external ventilation and heating in area's with high atmospheric dust loads (in that case use SR30)

Typical recommendations for use are:

- instrument cleaning interval < 7 days
- pyranometer calibration interval < 2 years

Exceptions to the recommendation are:

- when using Hukseflux model SR25: this model may be heated without using ventilation, still having low zero offsets.



**Figure 1** A typical problem in freezing conditions: ice accumulation on the pyranometer dome surface reduces data availability. At the front, a new pyranometer design with recirculating ventilation.

## Traditional external ventilation

The traditional solution is an external ventilation system as in Figure 3. Heated and ventilated air is blown over the pyranometer.

This ventilator:

- heats air and blows it over the pyranometer so that the dome is kept above dew point
- promotes thermal equilibrium between all components of radiometers, and thereby reduces zero offsets
- usually employs extra heaters because the ventilator heating power may not be enough
- often introduces additional thermal zero-offsets, in particular at high power heating. High power heating is only recommended if necessary

- consumes a lot of power because the heat is carried away by ventilation air; typically around 10 W
- requires regular maintenance of the ventilator and air filters
- is not recommended for use in area's with high atmospheric dust loads such as deserts with regular sand storms; rotating parts of ventilators tend to get stuck and are not designed to be cleaned
- does not reduce the pyranometer cleaning interval (reference ISO, WMO, BSRN, see below)
- does not reliably prevent snow or rain deposition on a dome

### New: SR30 with internal recirculating ventilation and heating


A new solution is internal recirculating ventilation. Internally heated and recirculated air keeps the instrument dome, above the dew point and at the same time it forces the body to the same temperature.

#### Internal ventilation:

- heats air and blows internally through the instrument so that the dome is above dew point
- makes sure the entire pyranometer is in thermal equilibrium, reducing zero offsets
- does not require extra heaters
- at high heating has no additional zero-offsets
- consumes low power because the heat is recirculated; 2 W consumption is normal
- requires replacement of the ventilator after > 5 years
- does not reduce the pyranometer cleaning interval (reference ISO, WMO, BSRN see below)
- does not reliably prevent snow or rain deposition on a dome

### Maintenance / cleaning

Ventilation is typically used with high accuracy measurement requirements. In such case the need for a high level of instrument maintenance and dome cleaning still exists; evaporating droplets of water might leave stains on the instrument domes. The bottom of external ventilation units usually provides access to the removable dust filter which needs regular cleaning.

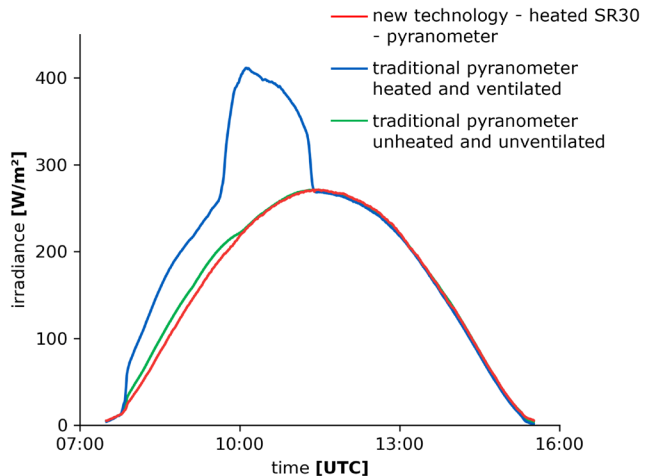

**Figure 2** Data availability in cold climates is negatively impacted by various factors. In this example, we examine a single rime event on a clear sky day in the Netherlands. SR30 is compared to two traditional pyranometers: one is unventilated and unheated while the other is externally ventilated and heated. On such a clear sky day, one expects a cosine-like curve such as the SR30 shows. Although the deviation of the unventilated pyranometer curve might be filtered out by data quality control, the deviation of the ventilated pyranometer curve can not be filtered out reliably, contaminating the data without you even knowing. Data taken on 4 DEC 2016, courtesy of KNMI.



**Figure 3** Traditional external VU01 ventilation unit with pyranometer SR20

## Generally recommended practices ISO TR9901 and ASTM G 183-05

ISO/TR 9901 "Solar Energy - Field Pyranometers - Recommended practice for use", recommends use of ventilators where high accuracy and reliability are required. It adds in 5.2.2 3 specific purposes:

- dew and frost formation are inhibited, especially from the outer dome,
- rain droplets on the outer dome are evaporated quickly, and
- the temperature of the instrument is maintained near to that of the ambient air.

Annex A1 adds: "Generally, pyranometers are ventilated continuously in order to provide a high level of reliability". More details can be found annex A2 which comments on different ventilation systems.

The maintenance schedule of pyranometers is described in chapter 5.2.3 and recommends daily cleaning of pyranometers, irrespective if they are ventilated or not.


ASTM G 183-05 "Standard Practice for field use of pyranometers, pyrhemometers and UV radiometers" is the ASTM equivalent of ISO TR9901.

In 5.3.2 it recommends daily inspection and cleaning of the instrument and a weekly check of operational state of the ventilator.

## IEC 61724-1: use for PV system performance monitoring

For class A and B systems you may use PV reference cells as well as pyranometers. According to table 5 pyranometers and PV reference cells must be heated. The purpose of the heating is mentioned in the same table: "to prevent accumulation of condensation and/or frozen precipitation", which is the main source of unreliable data in most climates. It is "required in locations where condensation and/or frozen precipitation would affect measurements on more than 7 days per year" for class A, and "more than 14 days per year" for class B. In class A systems only the pyranometers must be ventilated; the PV reference cells do not require ventilation because they do not suffer from zero offsets.

The IEC 61724- requires pyranometer "cleaning" also per table 5; at least once a week for Class A systems, once every 2 weeks for class B.

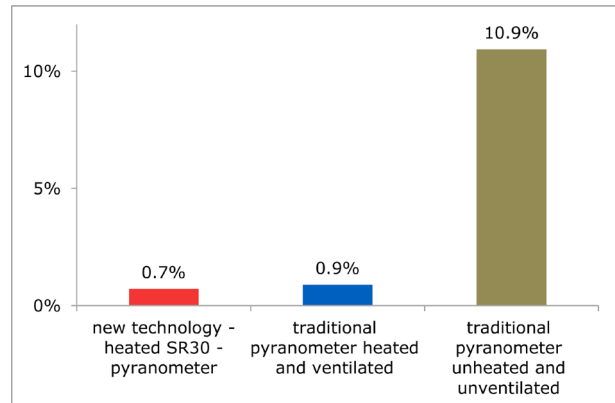

**Figure 4** Improving data availability by ventilation: on the vertical axis: unreliable data % of time. On our roof we analysed the data availability with an outdoor camera. We manually marked the moments that the pyranometer was covered with dew or frost. In autumn season with a traditional pyranometer (brown on the right) about 10 % of the time the data was not available. Because this was mainly in the early morning, this 10 % of time represented around 3 % of the total solar energy. With traditional external ventilation, the performance was much better, in blue around 1 %. With an SR30 with internal ventilation, in red, the performance is as good as with external ventilation.

## WMO: use in meteorological networks

About ventilation: in 7.3.3.5: "in some networks, the exposed dome of the pyranometer is ventilated continuously by a blower to avoid or minimize deposits in cold weather, and to cool the dome in calm weather situations. The temperature difference between the ventilating air and the ambient air should not be more than about 1 K. If local pollution or sand forms a deposit on the dome, it should be wiped very gently, preferably after blowing off most of the loose material or after wetting it a little, in order to prevent the surface from being scratched." About maintenance in 7.3.3: "It is most desirable that pyranometers and recorders be inspected at least daily, and preferably more often."

## BSRN: use with high accuracy diffuse radiation measurement

The Baseline Surface Radiation Network, BSRN, is a high quality network for climate change monitoring. It requires ventilation for all pyranometers in its BSRN operations manual v2.1.

In the BSRN network pyranometers are primarily used for measurement of diffuse irradiance. On a diffuse signal in the order of 200 W/m<sup>2</sup>, a zero

offset of the order of  $7 \text{ W/m}^2$  is very significant. Ventilation reduces this by a factor 2.

The primary purpose of ventilation in the BSRN network is reduction of zero offsets.

The BSRN manual in 4.2.2.1 recommends ventilation as a tool against zero offsets, dew, frost and snow. The manual says:

“The recommended procedures for the measurement of global radiation require the use of a ventilated housing to improve the overall stability of pyranometer measurement by damping changes in the pyranometer body temperature due to solar loading and potentially reducing the thermal offset. In some climates, the use of a ventilator also improves the amount of recoverable data by eliminating dew and reducing the number of occurrences of frost and snow on the instrument domes.

Locations where a ventilated housing are recommended are:

- where dew, frost or snow is prevalent,
- where natural ventilation is infrequent or variable,
- where there is significant radiative cooling during portions of the year, a ventilated housing may reduce thermal-offset,
- where the humidity is high during portions of the year a ventilator will reduce the possibility of water damage and reduce the frequency of desiccant changes”.

Maintenance schedule as described in chapter 6, recommends instrument cleaning as well as checks of the ventilator once per day, lubrication or cleaning of ventilators every year.



**Figure 5** Does ventilation work to remove snow? Not reliably: this photo shows 3 ventilation units in FEB 2014 in Logan UT, USA powder snow. Only 1 of the 3 pyranometers, the one at the right (SR20 with VU01), is visible. The other 2 are still covered in snow. Photo courtesy of Apogee Instruments Inc.

### About Hukseflux

Hukseflux Thermal Sensors offers measurement solutions for the most challenging applications. We design and supply sensors as well as test & measuring systems, and offer related services such as engineering and consultancy. Our main area of expertise is measurement of heat transfer and thermal quantities such as solar radiation, heat flux and thermal conductivity. Hukseflux is ISO 9001:2015 certified. Hukseflux sensors, systems and services are offered worldwide via our office in Delft, the Netherlands and local distributors.

Would you like more information?  
E-mail us at: [info@hukseflux.com](mailto:info@hukseflux.com)